


INSTALLATION INSTRUCTIONS Issue 1.0

FRONT PROTECTION COVERS DEGREE OF PROTECTION IP 65

Elastomeric material gasket with transparent plastic cover to achieve a degree of protection IP65 in installation of instruments with DIN 43700 enclosures. The gasket is inserted between the bezel edge of the measuring instrument and the exterior of the panel, being useful as well for fixing a transparent cover which protects the front part of the instrument.

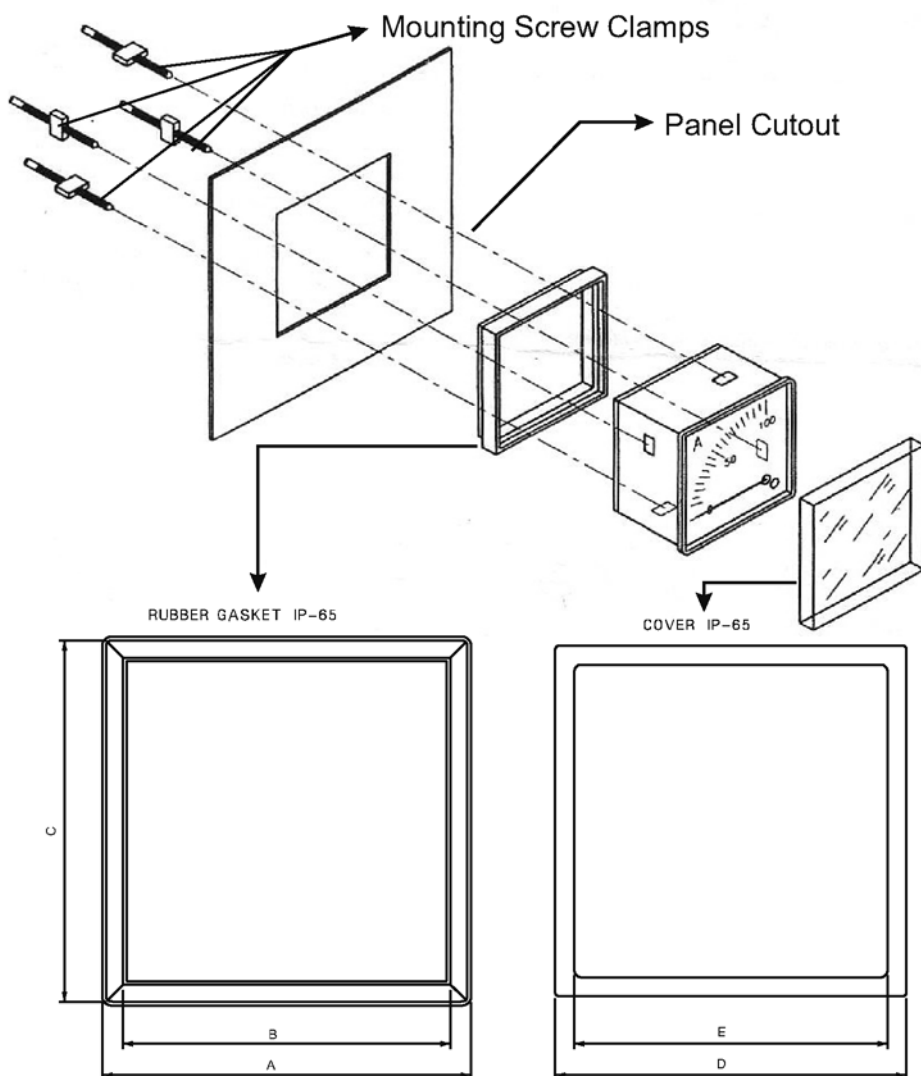

Its assembling is performed as follows:

1. Insert the instrument in the gasket.
2. It is recommended to apply a thin layer of silicone over the gasket side in contact with the external surface of the panel.
3. Insert the instrument and the gasket through the panel opening.
4. Hold by means of 4 fixing screw clamps from the back side of the panel, without tightening.
5. Using a screwdriver, insert the transparent cover between the bezel and the inner part of the gasket.
6. Tighten the 4 fixing screw clamps.

Panel Cutout Dimension As Per DIN 43700	
96x96 SIZE	□ 92 ^{+0.8}
72x72 SIZE	□ 68 ^{+0.7}
48x48 SIZE	□ 45 ^{+0.6}

IP-65 RUBBER GASKET			
	48	72	96
A	54.8	79.6	103.6
B	43.7	63.0	90.0
C	50.0	73.5	97.5
IP-65 COVER			
	48	72	96
D	50.2	74.6	98.6
E	39.5	64.0	88.0

* ALL DIM ARE IN mm.

Contact



Sifam Tinsley Instrumentation Ltd

1 Warner Drive
Springwood Industrial Estate
Braintree, Essex CM7 2YW

Tel: 01376 335271
E-mail: sales@sifamtinsley.com
www.sifamtinsley.co.uk

SUBJECT TO CHANGE WITHOUT NOTICE

This manual superseded all previous versions – please keep for future reference